

OPERATING INSTRUCTIONS




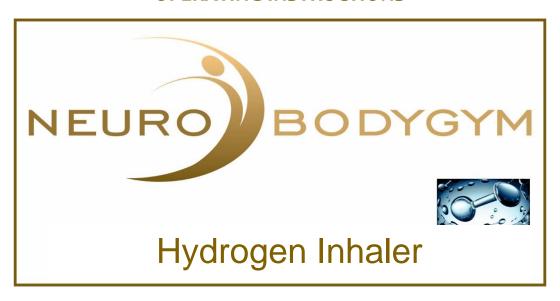



SetUp/Installation

Step 1: Preparation of the filter container

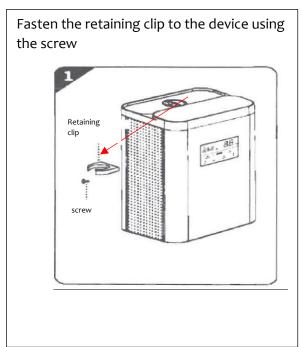


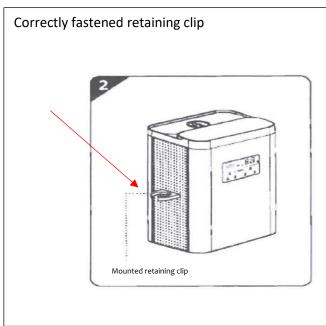

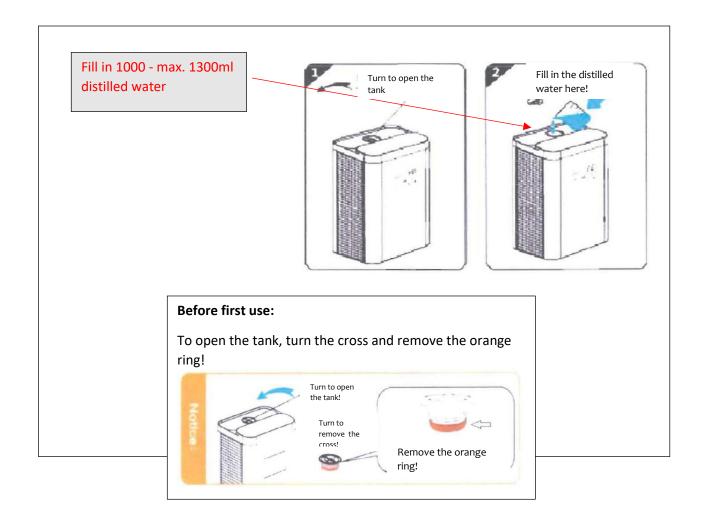


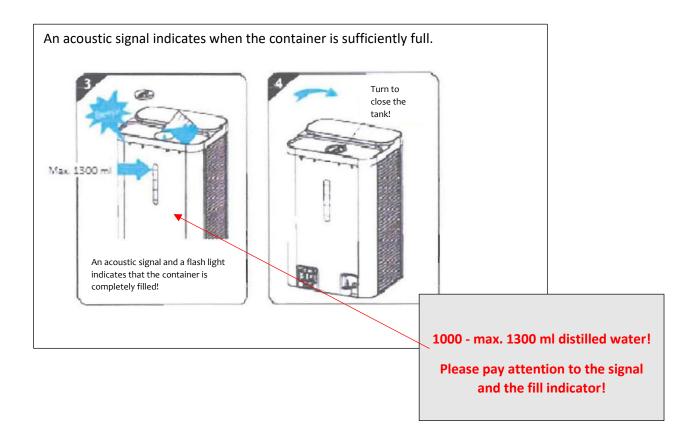


step 2: Preparation of the cannula-connection

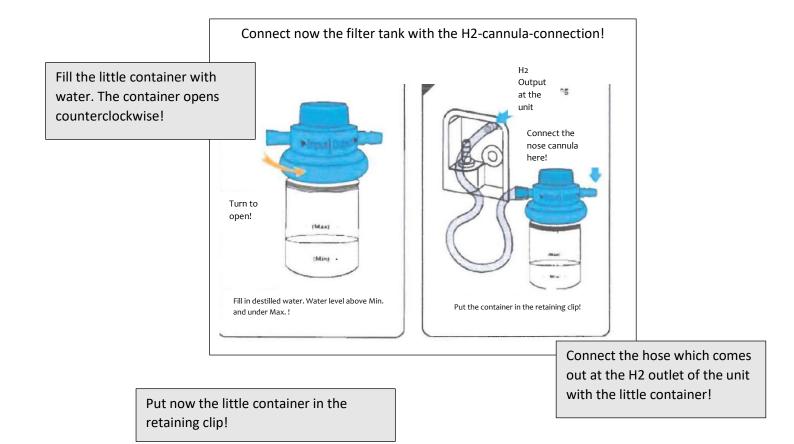


step 3:

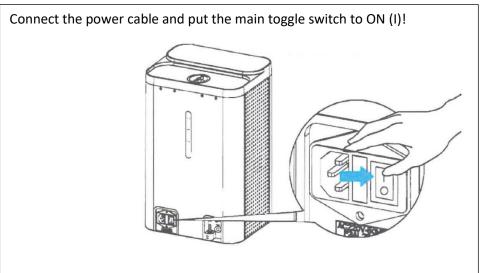


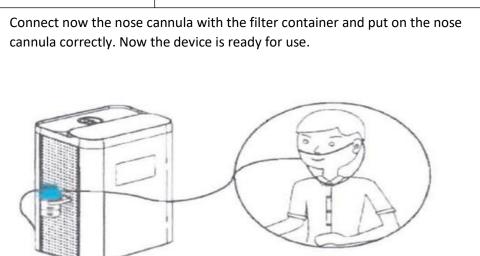

step 4: personalised use

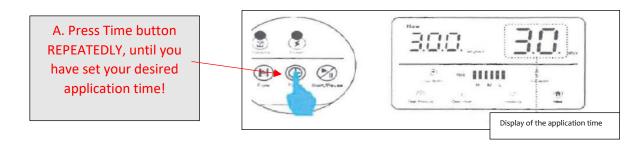

Select your individual application time, f.e. 30 minutes, 60 minutes or 2 hours etc.

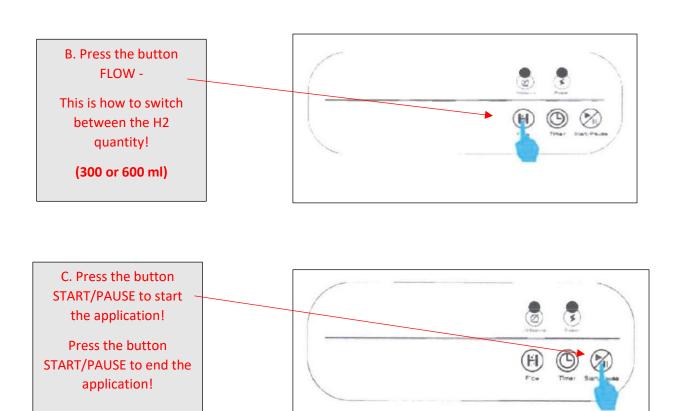



NeuroBodyTech GmbH, Waldstrasse 22, 83132 Pittenhart, managing director: Martin Rusam, Local Court München - HRB 241499 Tax Number.: 163/133/30102 (Finanzamt Traunstein), VAT-Nr.: DE320815970 EORI-Nr.: DE385010756645310 (Hauptzollamt Rosenheim)

Showroom & Data analysis: Seestrasse 39 (1. Stock), 83209 Prien am Chiemsee Technology & Software development: Bernauer Strasse 21 (1. Stock), 83209 Prien am Chiemsee Head office: Waldstrasse 22, 83132 Pittenhart im Chiemgau